


# Raman Analysis Of Active Compound vs. Placebo Sample Integration Through The Blister Pack

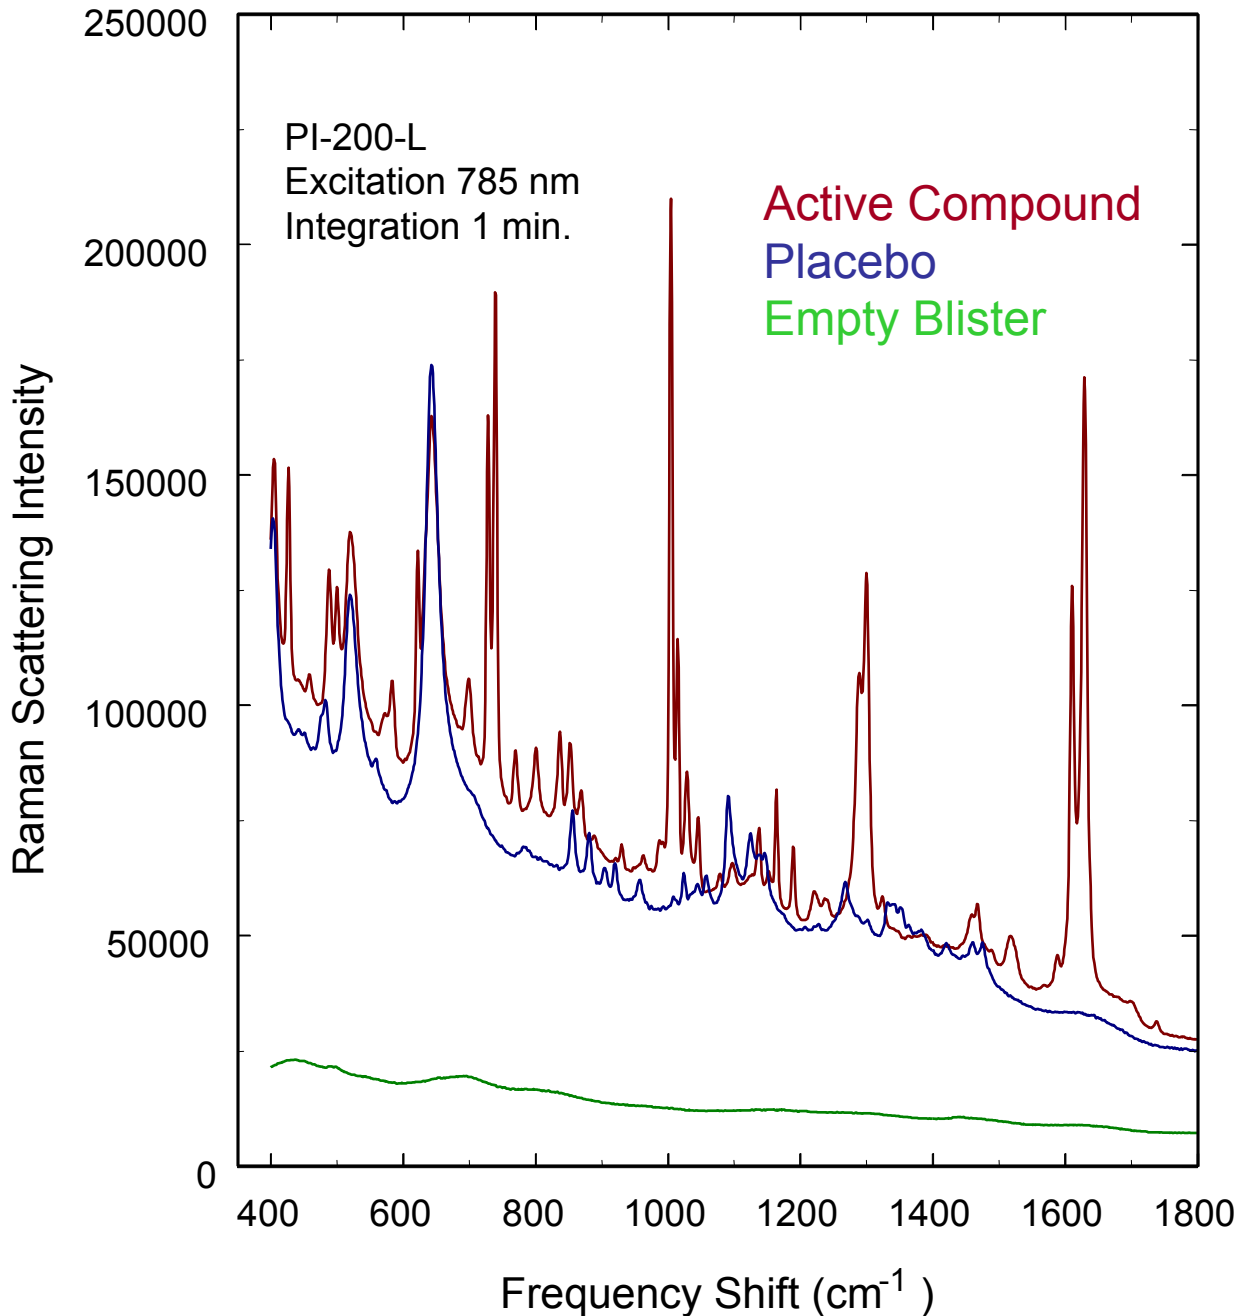

Spectral comparison between an active compound and a placebo where sample data acquisition was conducted through the blister pack. An empty blister pack spectrum is also displayed.